Keysight 8990B Peak Power Analyzer and N1923A/N1924A Wideband Power Sensors

Data Sheet





Faster Measurement Speed and Greater Measurement Accuracy

Skip the complicated setup and go straight to making measurements with the 8990B peak power analyzer from Keysight Technologies, Inc. This instrument offers faster measurement speed and greater measurement accuracy in key applications such as radar pulse analysis and wireless pulse measurement. Designed with both ease of use and high performance in mind, the 8990B peak power analyzer does more than just measure and analyze – it saves you time and effort, letting you focus on the important details.



Ease of use

8990B peak power analyzer is built for ease of use: the instrument is easy to set, easy to trigger and easy to measure pulse measurements with.

Setting	Set amplitude and time scale settings quickly with dedicated knobs and buttons, while the Autoscale function automatically displays waveforms scaled to the display. The function is accessible through a single touch button.
Trigger	Trigger the right pulse signal in three simple steps. Simply select the trigger source, the trigger edge and the trigger level, and the peak power analyzer will display the appropriate pulse signals.
Measure	Analyze a full range of parameters with 15 pulse parameter measurements, all pre-defined and executed automatically in two easy steps via the front panel touchscreen.


Additional features such as internal zero, calibration, and touchscreen capability make setup and data analysis both efficient and convenient, while a familiar button layout cuts the learning time needed to master using the instrument.

Performance

The 8990B peak power analyzer features a host of key performance specifications, dedicated to give you accurate and more detailed pulse measurements, faster.

Accuracy	Measure RF power measurements with less error; 8990B has an overall
	accuracy rate of 0.2 dB.
Detail	View pulses in greater image detail with the large 15-inch XGA color
	display and get the high resolution needed to detect abnormalities in a
	signal trace with the 8990B's sampling rate of 100 MSample/s (real time
	sampling) and 1 GSample/s (ETS mode).
Speed	Automatically execute pulse droop measurements for repetitive amplified
	pulse signals and delay measurement to detect the first pulse of the
	traces. The instrument's screen will instantly display the results.

And when combined with the N1923A/N1924A wideband power sensors, the 8990B achieves 5 nanosecond rise time/fall time – the fastest rise time/fall time in the peak power measurement market.

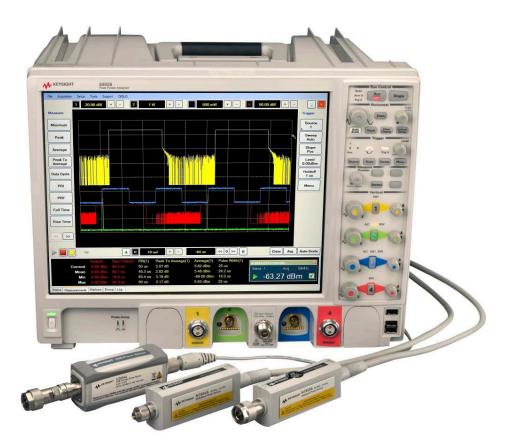

8990B Peak Power Analyzer Key Features




- Capture short radar pulses accurately with a 5 nanosecond overall rise time/fall time – the fastest rise time/fall time in the peak power measurement market – when the 8990B peak power analyzer is paired with the either the N1923A or N1924A wideband power sensor.
- A high sampling rate of 100 MSa/s lets you measure samples faster and view trace displays in high resolution.
- Analyze a full range of parameters with 15 pulse characterization measurements, including duty cycle, rise time, pulse top, pulse width, PRI and PRF.
- Verify design problems quickly with a 15-inch XGA color display that is capable of simultaneously displaying four channel results for more image detail, and manipulate data directly with a few touches of your finger with the touchscreen capability.
- Save time and eliminate inaccurate readings with the internal zero and calibration function.
- Continuously trigger and capture up to 512 pulses with the new multi-pulse measurement feature.
- Color coded channels allow you to pick out the channel data points of interest at a glance.
- Easily calculate the Power-Added Efficiency (PAE) of power amplifiers, and display instant PAE traces on the 8990B's display.
- Backwards compatibility with P-series sensors and U2000 series USB power sensors widens your sensor options and offers you an additional channel to the current four when a USB power sensor is connected. Download and install the N1918A Power Analysis Manager software to use the USB power sensor with the 8990B.

Graphical User Interface Overview




Measurement screen

The main measurement screen is capable of displaying up to four traces: two RF traces, and two video traces (the triggering signal). Results are shown in the panel directly under the graphical window, with measurements displayed in the same color as the channel to which it corresponds. When a USB sensor is connected, the results for this additional channel can be overlaid on the same graphical window in compact mode, The main screen also features a soft panel key to the side of the graphical window, which lists the 15 pulse characterization measurements for quick measurement analysis. Users can select these measurement parameters via the touchscreen display, or by using the mouse.



Delay measurement


Users can perform delay measurements by pressing the Delay Measurement button on the soft panel key. Two vertical markers will automatically detect the first pulse of the traces. The time delay between the two traces will be displayed in the measurement panel below the graphical window.



Droop measurement

The 8990B is the first peak power analyzer on the market that offers automated Pulse Droop measurement, eliminating the need to manually manipulate the horizontal markers to make this measurement. The Pulse Droop measurement is accessible via the soft panel key, and measures the amplitude degradation of the pulse top.

Graphical User Interface Overview (Continued)



Spacing measurement

Easily measure the space between pulses when a long pulse train occurs. The 8990B allows users to select the starting pulse and the end pulse, a function that is important in pulse block validation. R&D engineers may use this function to detect potential abnormalities in certain pulse groups, and whether those abnormalities are repeated in a long pulse train.



Zoom screen

The 8990B provides dual window zoom capability. When this function is enabled, the top screen will display the original signal, while the bottom screen displays the enlarged signal trace.

To focus and zoom in on a particular segment of the signal trace, use the white zoom box to select the area of interest on the original signal trace. The measurement panel below will display the results of the selected signal segment. This function provides R&D engineers the flexibility to focus on particular parts of the signal and to obtain only the measurement results they need.

The dual zoom window capability allows users to observe the original trace while focusing in on the selected signal segment instead of flipping between screens or losing the original trace after zooming in on the segment.

annel Seti	4P	×		cure Erape		89
1 2 2 0 4	need 1	Line (1)	4	trans onto	a antiroferen	1000000
Power Display : Scale :	105 7.05 dB		_	C CK	Cancel	
Frequency Ref Style : Centre Ref :	1 GHz CENTRE		Source	Chennel 1	M	Cost
ExtLoss: Bandwidth:	000 dB		Threeholds Power Mer Trace Ref!	automent	10%	Halp
30	eox Zerb	i	Trace Ref	Lui 2 (%) sion Ref Lui (%)	90%	7


Threshold/power display settings and erase memory

The 8990B allows users to change channel settings. The default threshold setting is 90% and 10%; however, users may change the reference levels to any value. If a pulse has high overshoot in the traces, users can choose to reduce the upper trace level to 80% or 70% to eliminate the overshoot signal's impact on the results. Users can also modify the trace level of two different signals for the delay measurement according to what is the best reference level for the individual signal.

Users can also change their settings to display power measurements in either logarithmic or watts to help with easy result conversion or to match the results to the traces in the graphical window.

For users in the aerospace and defense industry, the 8990B offers several ways to secure both data and measurement settings such as the memory sanitization feature, a standard product feature in all Keysight equipment that will erase the system's setup and data results. Users can also opt for the removable hard drive option, which switches the attached hard drive with a removable version, so users can remove data and settings together with the hard drive without worrying about information leaks.


Additional Features

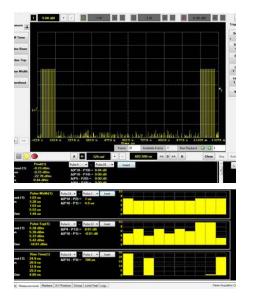

Multi-pulse measurement

View, measure and analyze continuous pulse trains from power amplifier modules or transmitters. The multi-pulse measurement feature allows continuously trigger and capture up to 512 pulses. This feature also adds pulse-to-pulse measurement and histogram distribution graph capabilities to the 8990B, which are crucial for testing RF and the pulse-to-pulse stability of power amplifiers and transmitters.


Additionally, operators can use the multi-pulse measurement feature to analyze short pulse with long off time or amplitude droop across the pulse train, or monitor the stability of the pulse shape (via the histogram graph functionality).



Power-Added Efficiency math function

Calculate the Power-Added Efficiency (PAE) of power amplifiers and display instant PAE traces onscreen with the 8990B. Power-Added Efficiency, a typical power analyze measurement, is a measure of the power conversion efficiency – the percentage of DC power converted to RF power in the power amplifier – of power amplifiers.

Reduce test costs and the number of test equipment needed with the 8990B; the peak power analyzer measures RF power, voltage and current in a single solution box. The 8990B's two RF input channels allow users to measure the RF power gain from the power amplifier; using a DC current probe, scope probe or differential probe, they can also measure the power amplifier's voltage and current through the analog video input channels. The 8890B's PAE math function then uses the measurements from the RF and analog video input channels to easily determine the PAE of the power amplifier.

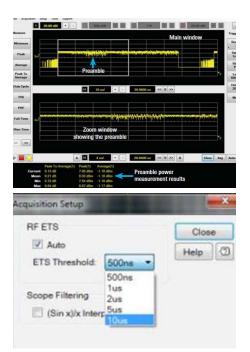

Adjustable ETS threshold for wider bandwidth measurement

Measure peak and peak-to-average of 802.11ac wide bandwidth signal accurately with the 8990B's 160 MHz video bandwidth capability. The peak power analyzer can execute power vs. time (PvT) measurements on an 80 MHz or 160 MHz 802.11ac signal by adjusting the ETS threshold according to the burst length.

Operators can also use the zoom function to analyze and measure the preamble power of the 802.11ac burst signal.

Performance Specifications

Specification definitions

There are two types of product specifications:

- Warranted specifications are specifications which are covered by the product warranty and apply over a range of 0 to 55 °C unless otherwise noted. Warranted specifications include measurement uncertainty calculated with a 95% confidence.
- **Characteristic specifications** are specifications that are not warranted. They describe product performance that is useful in the application of the product. These characteristic specifications are shown in *italics*.

Characteristic information is representative of the product. In many cases, it may also be supplemental to a warranted specification. Characteristic specifications are not verified on all units. There are several types of characteristic specifications. They can be divided into two groups:

One group of characteristic types describes 'attributes' common to all products of a given model or option. Examples of characteristics that describe 'attributes' are the product weight and '50-ohm input Type-N connector'. In these examples, product weight is an 'approximate' value and a 50-ohm input is 'nominal'. These two terms are most widely used when describing a product's 'attributes'.

Conditions

The power meter and sensor will meet its specifications when:

- Stored for a minimum of two hours at a stable temperature within the operating temperature range, and turned on for at least 30 minutes.
- The power meter and sensor are within their recommended calibration period.
- Used in accordance to the information provided in the User's Guide.

Product Characteristics

The following specifications are applicable only when the N1923A/N1924A wideband power sensors are used with the 8990B peak power analyzer. Using the 8990B with other supported sensors might yield different results.

Power requirements	100 to 120 V (at 50 to 60 Hz, 400 Hz)
i olioi roqui olionici	100 to 240 V (at 50 to 60 Hz)
	Maximum power dissipated at 375 W
Operating environment	Operating temperature from 5 to 40 °C
	Relative humidity up to 95% at 40 °C (non-condensing)
	Operating altitude up to 4000 m (12000 ft.)
	Operating random vibration at 5 to 500 Hz, 10 minutes/axis, 0.21 g (rms)
Non-operating conditions	Non-operating temperature from –40 to +70 °C
	Relative humidity up to 90% at 65 °C
	Non-operating altitude up to 4600 m (15000 ft.)
	Non-operating random vibration at 5 to 500 Hz, 10 minutes/axis, 2.09 g (rms); resonant search at 5 to 500 Hz, swept
	sine, 1 octave/minute, sweep rate at 0.5 g (0 peak), 5 minutes resonant, dwell at 4 resonance/axis
Dimensions (W x D x H)	430 mm (16.9 in) x 347 mm (13.7 in) x 330 mm (13.0 in)
Weight	< 16 kg (net)
	< 23.5 kg (shipping)
Sound pressure level	45 dB
Electromagnetic	Complies with the essential requirements of the European (EC) Directives as follows:
compatibility	- IEC 61326-2-1:2005/EN 61326-2-1:2006
	– CISPR 11:2003/EN 55011:2007 (Group 1, Class A)
	The product also meets the following EMC standards:
	– Canada: ICES-1:2004
	 Australia/New Zealand: AS/NZS CISPR 11:2004
Safety	Conforms to the following product specifications:
	– EN61010-1: 2001/IEC 61010-1:2001
	– CAN/CSA C22.2 No. 61010-1-04
	 ANSI/UL std No. 61010-1-2004

8990B Peak Power Analyzer Specifications

Key specifications			
RF input channels	2		
Video input channels	2		
Maximum real time sampling rate	100 MSa/s ¹ (Real Time), 1 GSa/s ¹ (ETS On), 20 GSa/s ²		
Maximum capture length	1 s		
Memory depth	Max 2M points		
Instrumentation linearity	± 0.8%		
Rise time/fall time	≤ 5 nsec (for frequencies ≥ 500 MHz) ³		
RF inputs (Channels 1 and 4)			
Frequency range	50 MHz to 40 GHz		
Dynamic range	–35 dBm to +20 dBm		
Measurement unit	Linear (Watt) or Log (dBm) selectable		
Video bandwidth	160 MHz ⁴		
Minimum pulse width	50 ns		
Maximum pulse repetition rate	10 MHz		
Input coupling	50 Ω		
Vertical scale	0.01 dB/div to 100 dB/div in 1-2-5 sequence	or any arbitrary scaling, user defined	
	1 μW/div to 1 kW/div in 1-2-5 sequence or ar	ny arbitrary scaling, user defined	
Offset	± 99 dBm with 0.01 dB resolution		
ETS threshold	500 ns, 1 μs, 2 μs, 5 μs, 10 μs		
Video inputs (Channels 2 and 3)			
General characteristics			
Video bandwidth	1 GHz		
Input impedance	$50 \ \Omega \pm 2.5\%$, 1 M $\Omega \pm$ 1% (11 pF typical)		
Input coupling	1 MΩ: AC (3.5 Hz), DC		
	50 Ω: DC		
Vertical scale	1 MΩ: 1 mV/div to 5 V/div in 1-2-5 sequence o	r any arbitrary scaling, user defined	
	50 Ω : 1 mV/div to 1 V/div in 1-2-5 sequence or	any arbitrary scaling, user defined	
DC gain accuracy	± 2% of full scale at full resolution on channel		
Offset accuracy	± (1.25% of channel offset +1% of full scale + 1	1 mV) ⁵	
Maximum input voltage	1 MΩ: 150 V RMS or DC, CAT I		
	± 250 V (DC + AC) in AC coupling		
Offset range			
	Vertical sensitivity	Available offset	
1 ΜΩ	1 mV to < 10 mV/div	± 2 V	
	10 mV to < 20 mV/div	± 5 V	
	20 mV to < 100 mV/div	± 10 V	
	100 mV to < 1 V/div	± 20 V	
	1 V to 5 V/div	± 100 V	
50 Ω		± 12 div or ± 4 V, whichever is smallest	

1. For RF input channel 1 and 4.

2. For video input channel 2 and 3.

3. Specification applies only when the Off video bandwidth is selected.

4. Video bandwidth tested by measuring peak-to-average on a two-tone separation signal at +10 dBm, frequency set at 1 GHz. Test limit set at 2 dB roll off from the nominal 3 dB peak-to-average flatness graph.

5. 50 Ω input: Full scale is defined as 8 vertical divisions. Magnification is used below 10 mV/div, full-scale is defined as 80 mV. The major scale settings are 5 mV, 10 mV, 20 mV, 500 mV, 200 mV, 500 mV, and 1 V.

1 MΩ input: Full scale is defined as 8 vertical divisions. Magnification is used below 5 mV/div, full-scale is defined as 40 mV. The major scale settings are 5 mV, 10 mV, 20 mV, 50 mV, 100 mV, 200 mV, 500 mV, 1 V, 2 V, and 5 V.

8990B Peak Power Analyzer Specifications (Continued)

Time base	
Range	2 ns to 100 msec/div in 1-2-5 sequence or any arbitrary scaling, user defined
Delta time accuracy	1 ns + 0.02 x (time/div)
Timebase accuracy	± 1.4 ppm peak
Channel to channel offset	± 5 ns (ETS Off), ± 3 ns (ETS On)
Delay range	±1smax
Trigger	
Hardware trigger	
Sweep mode	Auto, triggered, single
Trigger mode	Postive and negative edge, pulse width (all channels)
	Trigger by event (sensor channel 1 and 4)
Trigger source	Channel 1, 2, 3, 4, AUX
Trigger level	
Level range	Channel 1 and 4: –20 dBm to +20 dBm
0	Channel 2 and 3: \pm 8 div from center screen (1 M Ω , edge mode)
	AUX: TTL (high > 2.4 V, low < 0.7 V at 50 Ω
Level resolution	Channel 1 and 4: 0.01 dB
	Channel 2 and 3: 10 μ V ¹
Level accuracy	Channel 1 and 4: ± 0.5 dB (0.5 dB/ns slew rate in ETS mode)
Trigger delay	
Delay range	± 1.0 s max ²
Delay resolution	1% of delay setting, 10 ns maximum (50 ns/div)
Trigger hold-off	
Range	1 µs to 1 s
Resolution	1% of selected value (to a minimum of 10 ns)
Vertical and horizontal markers	
Resolution	Minimum 1 ns
Sensor check source	
Frequency	1.05 GHz or 50 MHz (selectable)
Power level	0 dBm ± 0.9% (50 MHz)
	0 dBm ± 1.2% (1.05 GHz)
Signal type	Square pulse modulated (1.05 GHz only) or CW (1.05 GHz or 50 MHz)
Repetition rate	1 kHz
Connector type	Type N (female)
SWR	1.05
Waveform measurement and math	
Pulse measurement	Rise time, fall time, minimum, average, peak, peak-to-average, duty cycle, PRI, PRF, off time, pulse base, pulse top,
	pulse width, overshoot
Markers measurement	Delay measurement, pulse spacing, pulse droop
Waveform math	Add, averaging, common mode, divide, invert, magnify, multiply, PAE, PAE2, subtract, square root, XY display
Statistical	CCDF (free run and triggered)
Video averaging	2, 4, 8, 32, 64, 128, 256, 512, 1024, 2048 selectable
Zoom	Dual window zoom

The trigger level of video channels is dependent on the vertical scale setting.
 The trigger delay range is dependant on the timebase setting.

8990B Peak Power Analyzer Specifications (Continued)

Multi-pulse specifications	
Maximum capture frame	512 (each channel 1 and channel 4)
Minimum pulse to pulse duration	1μs
Number of histogram bins	20 (user adjustable)
Pulse to Pulse measurement	Compare any two pulses from the captured frames
Sensor compatibility	
N1921A	P-Series wideband power sensor, 50 MHz to 18 GHz
N1922A	P-Series wideband power sensor, 50 MHz to 40 GHz
N1923A	Wideband power sensor, 50 MHz to 18 GHz
N1924A	Wideband power sensor, 50 MHz to 40 GHz
Computer system and peripherals, I/	'O ports
Display	
Display	15-inch color XGA TFT-LCD with touchscreen capability
Computer system and peripherals	
Operating system	Windows 7 Embedded Standard
СРИ	Intel Core 2TM Duo CPU E8400 3 GHz microprocessor
System memory	4 GB
Drives	$ m \geq 250~GB$ internal hard disk (option 800)
	\ge 250 GB removable hard disk (option 801)
Peripherals	Optical USB mouse and compact keyboard supplied.
	Supports any Windows compatible input device with a PS/2 or USB interface.
File types	
Waveforms	Comma separated values (*.csv)
mages	BMP, TIFF, GIF, PNG or JPEG
/O ports	
LAN	RJ-45 connector, supports 10Base-T, 100Base-T and 1000Base-T. Enables web-enabled remote control, e-ma
	on trigger, data/file transfers and network printing.
RS-232 (serial)	COM1, printer and pointing device support
PS/2	Two ports. Supports PS/2 pointing and input devices.
JSB 2.0 Hi-Speed	Three ports (front panel)
	Four ports (side panel)
	Allows connection of USB peripherals like storage devices and pinitng devices while the peak power analyzer is
	turned on. One device port on the side.
Dual-monitor video output	15-pin XGA on side, full color output of scope waveform display or dual monitor video output
Auxiliary output	DC (± 2.4 V); square wave ~755 Hz with ~200 ps rise time
Trigger out	Output provides TTL compatible logic levels and uses a BNC connector
Fime base reference output	10 MHz, amplitude into 50 Ω , 800 m Vpp to 12.6 Vpp (4 dBm ± 2 dB) if derived from internal reference.
	Tracks external reference input amplitude ± 1 dB if applied and selected.
Time base reference input	10 MHz, input Z = 50 Ω
	Minimum, –2 dBm
	Maximum, +10 dBm
Remote programming	
nterface	LAN and USB 2.0 interface
Command language	SCPI

N1923A/N1924A Wideband Power Sensor Specifications

Sensor model	Frequency range	Dynamic range	Rise/fall time	Damage level	Connector type
N1923A	50 MHz to 18 GHz	–35 to +20 dBm	≤ 3 ns (applicable for	+23 dBm (average power);	Type N (m)
			frequencies of ≥ 500 MHz)	+30 dBm (< 1 µs duration, peak power)	
N1924A	50 MHz to 40 GHz	–35 to +20 dBm	≤ 3 ns (applicable for	+23 dBm (average power);	2.4 mm (m)
			frequencies of ≥ 500 MHz)	+30 dBm (< 1 µs duration, peak power)	

The N1921A/N1922A P-series wideband power sensors are compatible for use with the 8990B peak power analyzer.

Maximum SWR

Frequency band	N1923A	N1924A
50 MHz to 10 GHz	1.2	1.2
10 GHz to 18 GHz	1.26	1.26
18 GHz to 26.5 GHz		1.3
26.5 GHz to 40 GHz		1.5

Sensor calibration uncertainty ¹

Frequency band	N1923A	N1924A
50 MHz to 500 MHz	4.5%	4.3%
500 MHz to 1 GHz	4.0%	4.2%
1 GHz to 10 GHz	4.0%	4.4%
10 GHz to 18 GHz	5.0%	4.7%
18 GHz to 26.5 GHz		5.9%
26.5 GHz to 40 GHz		6.0%
Physical characteristics		
Dimensions	N1923A	135 mm x 40 mm x 27 mm (5.3 in x 1.6 in x 1.1 in)
	N1924A	127 mm x 40 mm x 27 mm (5.0 in x 1.6 in x 1.1 in)
Weights with cable	Option 105	0.4 kg (0.88 lb)
	Option 106	0.6 kg (1.32 lb)
Fixed sensor cable lengths	Option 105	1.5 m (5-feet)
	Option 106	3.0 m (10-feet)

Environmental conditions

General	Complies with the requirements of the EMC Directive 89/336/EEC
Operating	
Temperature	0 to 55 °C
Maximum humidity	95% at 40 °C (non-condensing)
Minimum humidity	15% at 40 °C (non-condensing)
Maximum altitude	3,000 meters (9,840 feet)
Storage	
Non-operating storage temperature	-30 to +70 °C
Non-operating maximum humidity	90% at 65 °C (non-condescending)
Non-operating maximum altitude	15,420 meters (50,000 feet)

1. Beyond 70% humidity, an additional 0.6% should be added to these values.


System Specifications and Characteristics

Average power measurement accuracy		
N1923A	$\leq \pm 0.2 \ dB \ or \pm 4.5\%^{-1}$	
N1924A	$\leq \pm 0.3 dB \text{or} \pm 6.7\%$	

1. Specification is valid over a range of -15 to +20 dBm, and a frequency range of 0.5 to 10 GHz, DUT Max. SWR < 1.27 for the N1923A, and a frequency range of 0.5 to 40 GHz, DUT Max. SWR < 1.2 for the N1924A. Averaging is set to 32.

Video bandwidth

The video bandwidth in the peak power analyzer can be set to High, Medium, Low and Off. The video bandwidths stated in the table below are not the 3 dB bandwidths, as the video bandwidths are corrected for optimal flatness (except the Off filter). Refer to Figure 1 for information on the flatness response. The Off video bandwidth setting provides the warranted rise time and fall time specification and is the recommended setting for minimizing overshoot on pulse signals.

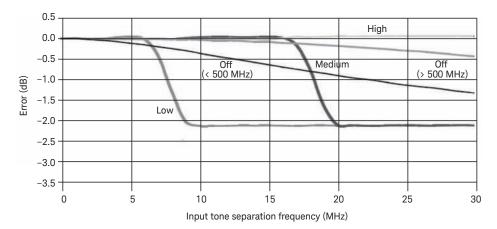



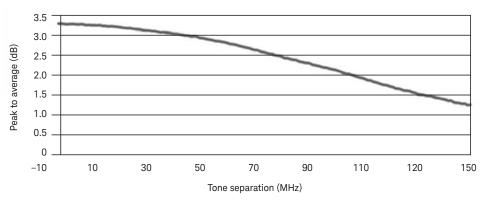


Figure 2. Video Bandwidth set to Off.

System Specifications and Characteristics (Continued)

Dynamic response - ri	se time, fal	ll time, and	overshoot v	ersus video	bandwidth s	ettings	6					
	Video ba	andwidth se	etting									
Parameter	Low: 5 MHz		Mediun	Medium: 15 MHz		High: 30 MHz		Off				
							< 500 MHz	> 500	MHz			
Rise time/Fall time ¹	< 60 ns		< 25 ns		< 13 ns		< 50 ns	≤ 5.5	ns			
Overshoot ²							< 5%	< 5%				
Noise and drift ³												
Sensor model	Zeroing		Zero se	Zero set			Zero drift ⁴	Noise	Noise per sample		Measurement noise ⁵	
			< 500 I	< 500 MHz		> 500 MHz						
N1923A/N1924A	No RF on input		200 nW 200 nW		200 nW		80 nW 3 μW		50 nW			
	RF present		550 nW		200 nW	200 nW 80 nW		3 μW		50 nW		
Noise per sample mul	tiplier				•							
	•	andwidth se	etting									
	Low: 5 MHz Medium: 15 MH		/Hz		High: 30 MHz		Off					
< 500 MHz	0.91				1		1					
> 500 MHz	0.56		0.74			0.93		1				
Noise multiplier												
Average setting	1	2	4	8	16	32	64	128	256	512	1024	
< 500 MHz	1.00	0.75	0.55	0.40	0.35	0.30	0.25	0.22	0.21	0.20	0.19	
> 500 MHz	1.00	0.73	0.52	0.37	0.28	0.21	0.17	0.15	0.14	0.14	0.14	

Dynamic response - rise time, fall time, and overshoot versus video bandwidth settings

1. Specified as 10 to 90% for rise time and 90 to 10% for fall time on a 0 dBm pulse.

2. Specified as the overshoot relative to the settled pulse top power.

3. In triggered mode with timebase setting at 4 msec/div.

4. Within 1 hour after a zero, at a constant temperature, after 24 hours warm-up of the peak power analyzer. This component can be disregarded with Autozero mode set to ON.

5. Measured over a one-minute interval, at a constant temperature, two standard deviations, with averaging set to 1.

Effect of video bandwidth setting

The noise per sample is reduced by applying the meter video bandwidth filter setting (High, Medium or Low). If averaging is implemented, this will dominate any effect of changing the video bandwidth.

Effect of time-gating on measurement noise

The measurement noise on a time-gated measurement will depend on the time gate length. 100 averages are carried out every 1 μ s of gate length. The Noise-per-Sample contribution in this mode can approximately be reduced by $\sqrt{\text{gate length/10 ns}}$ to a limit of 50 nW.

16 | Keysight | 8990B Peak Power Analyzer and N1923A/N1924A Wideband Power Sensors - Data Sheet

Appendix A

Uncertainty calculations for a power measurement (settled, average power)

[Specification values from this document are in **bold**, values calculated on this page are <u>underlined</u>.]

Process

1.	Power level	W			
2.	Frequency				
3.	Calculate meter uncertainty:				
	Calculate noise contribution Noise = Noise-per-sample x noise per sample multiplier				
	Convert noise contribution to a relative term ¹ = <u>Noise/Power</u>	%			
	Instrumentation linearity	%			
	Drift	%			
	RSS of above three terms ≥ <u>Meter uncertainty</u> =	%			
4.	Zero uncertainty (Mode and frequency-dependent) = Zero set/ <u>Power</u> =	%			
5.	Sensor calibration uncertainty (Sensor, frequency, power and temperature-dependent) =	%			
6.	System contribution, coverage factor of $2 \ge sys_{rss} = \dots$ (RSS three terms from steps 3, 4 and 5)	%			
7.	Standard uncertainty of mismatch				
	Max SWR (frequency-dependent) =	%			
	Convert to reflection coefficient, $ \rho_{\text{Sensor}} = (\text{SWR-1})/(\text{SWR+1}) = \dots$	%			
	Max DUT SWR (frequency-dependent) =	%			
	Convert to reflection coefficient, $\mathbf{\rho}_{_{\mathrm{DUT}}}$ = (SWR–1)/(SWR+1) =	%			
8.	Combined measurement uncertainty @ k=1				
	$U_{\rm C} = \sqrt{\left(\frac{{\rm Max}(\boldsymbol{\rho}_{\rm DUT}) \bullet {\rm Max}(\boldsymbol{\rho}_{\rm Sensor})}{\sqrt{2}}\right)^2 + \left(\frac{{\rm Sys}_{\rm rss}}{2}\right)^2} \qquad \dots$	%			
	Expanded uncertainty, k = 2, = UC • 2 =	%			

1. The noise-to-power ratio is capped for powers > 100 $\mu\text{W},$ in these cases use: Noise/100 $\mu\text{W}.$

17 | Keysight | 8990B Peak Power Analyzer and N1923A/N1924A Wideband Power Sensors - Data Sheet

Worked Example

Uncertainty calculations for a power measurement (settled, average power)

[Specification values from this document are in **bold**, values calculated on this page are underlined.]

Process

1.	Power level	1 mW				
2.	Frequency	1 GHz				
3.	Calculate meter uncertainty:					
	Calculate noise contribution Noise = Noise-per-sample x noise per sample multiplier = 3 μW x 1					
	Convert noise contribution to a relative term1 = $Noise/Power = 3 \mu W/1 m W$	0.3%				
	Instrumentation linearity	0.8%				
	Drift					
	RSS of above three terms ≥ <u>Meter uncertainty</u> =	0.85%				
4.	Zero uncertainty (Mode and frequency-dependent) = Zero set/ <u>Power</u> = 200 nW/1 mW	0.02%				
5.	Sensor calibration uncertainty (Sensor, frequency, power and temperature-dependent) =	4.0%				
6.	System contribution, coverage factor of $2 \ge sys_{rss} = \dots$ (RSS three terms from steps 3, 4 and 5)	4.09%				
7.	Standard uncertainty of mismatch					
	Max SWR (frequency-dependent) =	1.2%				
	Convert to reflection coefficient, $ \rho_{\text{Sensor}} = (\text{SWR-1})/(\text{SWR+1}) =$	0.091%				
	Max DUT SWR (frequency-dependent) =	1.26%				
	Convert to reflection coefficient, $ \rho_{DUT} = (SWR-1)/(SWR+1) =$	0.115%				
8.	Combined measurement uncertainty @ k=1					
	$U_{\rm C} = \sqrt{\left(\frac{{\rm Max}({\bf \rho}_{\rm DUT}) \bullet {\rm Max}({\bf \rho}_{\rm Sensor})}{\sqrt{2}}\right)^2 + \left(\frac{{\rm Sys}_{\rm rss}}{2}\right)^2} \qquad \dots$	2.045%				
	Expanded uncertainty, k = 2, = UC • 2 =	4.09%				

1. The noise-to-power ratio is capped for powers > 100 μ W, in these cases use: Noise/100 μ W.

Ordering Information

	Model	Description				
Meter	8990B	Peak power analyzer				
Standard-shipped	Optical mouse					
accessories	Stylus pen					
	Mini keyboard					
	Calibration certificate					
	IO libraries media suite					
	50 Ω BNC cable					
Sensor	N1923A	Wideband power sensor, 50 MHz to 18 GHz				
	N1924A	Wideband power sensor, 50 MHz to 40 GHz				
Standard-shipped	Calibration certificate					
accessories	N1923A/N1924A wideband power sensor operating and service guide - English					
	Options	Description				
Meter	8990B-800	Standard hard drive, installed				
	8990B-801	Removable hard drive, installed				
	8990B-U01	With USB host				
	8990B-U02	Without USB host				
Sensors	N1923A-105	Fixed cable option length, 1.5 m (5 ft)				
00.0010	N1923A-106	Fixed cable option length, 3 m (10 ft)				
	N1924A-105	Fixed cable option length, 1.5 m (5 ft)				
	N1924A-106	Fixed cable option length, 3 m (10 ft)				
Other accessories	8990B-1CM	Rackmount kit, 8U full rack				
	N6921A	Stacking kit				
	N6922A	BNC extension cable, male to female				
	N6923A	BNC adapter, right angle				
	N6924A	Additional hard drive with image				
	N6925A	Storage pouch				
Warranty and calibration	8990B-1A7	Compliant calibration test data - ISO17025, printed				
wallality allu calibration	8990B-A6J	Certificate of compliance calibration - ANSI/NCSL Z540, printed				
	N1923A-1A7	Certificate of compliance calibration - ISO 17025 with test data; printed				
	N1923A-A6J	Certificate of compliance calibration - ANSI Z540 with test data; printed				
	N1923A-A03	Certificate of compliance calibration - ISO 17025 with test data; printed				
	N1924A-A6J	Certificate of compliance calibration - ANSI Z540 with test data; printed				
Documentation	8990B-0BF	English language programming guide, printed				
Documentation	8990B-0BK	English language user and programming guide, printed				
	8990B-0BW	English language service guide, printed				
	8990B-ABJ					
		Japanese user guide and English programming guide, printed Do not include printed manuals				
	8990B-0B0					
	8990B-ABA	English language user guide, printed				
	N1923A-ABJ	Japan, Japanese user guide, printed				
	N1923A-0B1	English language user guide, printed				
	N1924A-ABJ	Japan, Japanese user guide, printed				
	N1924A-0B1	English language user guide, printed				
	N1923A-OBN	English language service guide, printed				
0 - (1	N1924A-0BN	English language service guide, printed				
Software	8990B-1FP	Multi-pulse analysis software, fixed perpetual license				
	N6903A	Multi-pulse analysis software				

myKeysight

Three-Year Warranty

Keysight Assurance Plans

myKeysight

www.keysight.com/find/mykeysight

A personalized view into the information most relevant to you.



www.keysight.com/find/ThreeYearWarranty

Keysight's commitment to superior product quality and lower total cost of ownership. The only test and measurement company with three-year warranty standard on all instruments, worldwide.



www.keysight.com/find/AssurancePlans

Up to five years of protection and no budgetary surprises to ensure your instruments are operating to specification so you can rely on accurate measurements.



www.keysight.com/go/quality

Keysight Technologies, Inc. DEKRA Certified ISO 9001:2008 Quality Management System

Keysight Channel Partners

www.keysight.com/find/channelpartners

Get the best of both worlds: Keysight's measurement expertise and product breadth, combined with channel partner convenience.

www.keysight.com/find/peakpoweranalyzer

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

Americas

Canada	(877) 894 4414
Brazil	55 11 3351 7010
Mexico	001 800 254 2440
United States	(800) 829 4444

Asia Pacific

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 112 929
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 6375 8100

Europe & Middle East

Austria	0800 001122
Belgium	0800 58580
Finland	0800 523252
France	0805 980333
Germany	0800 6270999
Ireland	1800 832700
Israel	1 809 343051
Italy	800 599100
Luxembourg	+32 800 58580
Netherlands	0800 0233200
Russia	8800 5009286
Spain	800 000154
Sweden	0200 882255
Switzerland	0800 805353
	Opt. 1 (DE)
	Opt. 2 (FR)
	Opt. 3 (IT)
United Kingdom	0800 0260637

For other unlisted countries: www.keysight.com/find/contactus (BP-09-23-14)



This information is subject to change without notice. © Keysight Technologies, 2013 - 2015 Published in USA, April 8, 2015 5990-8126EN www.keysight.com